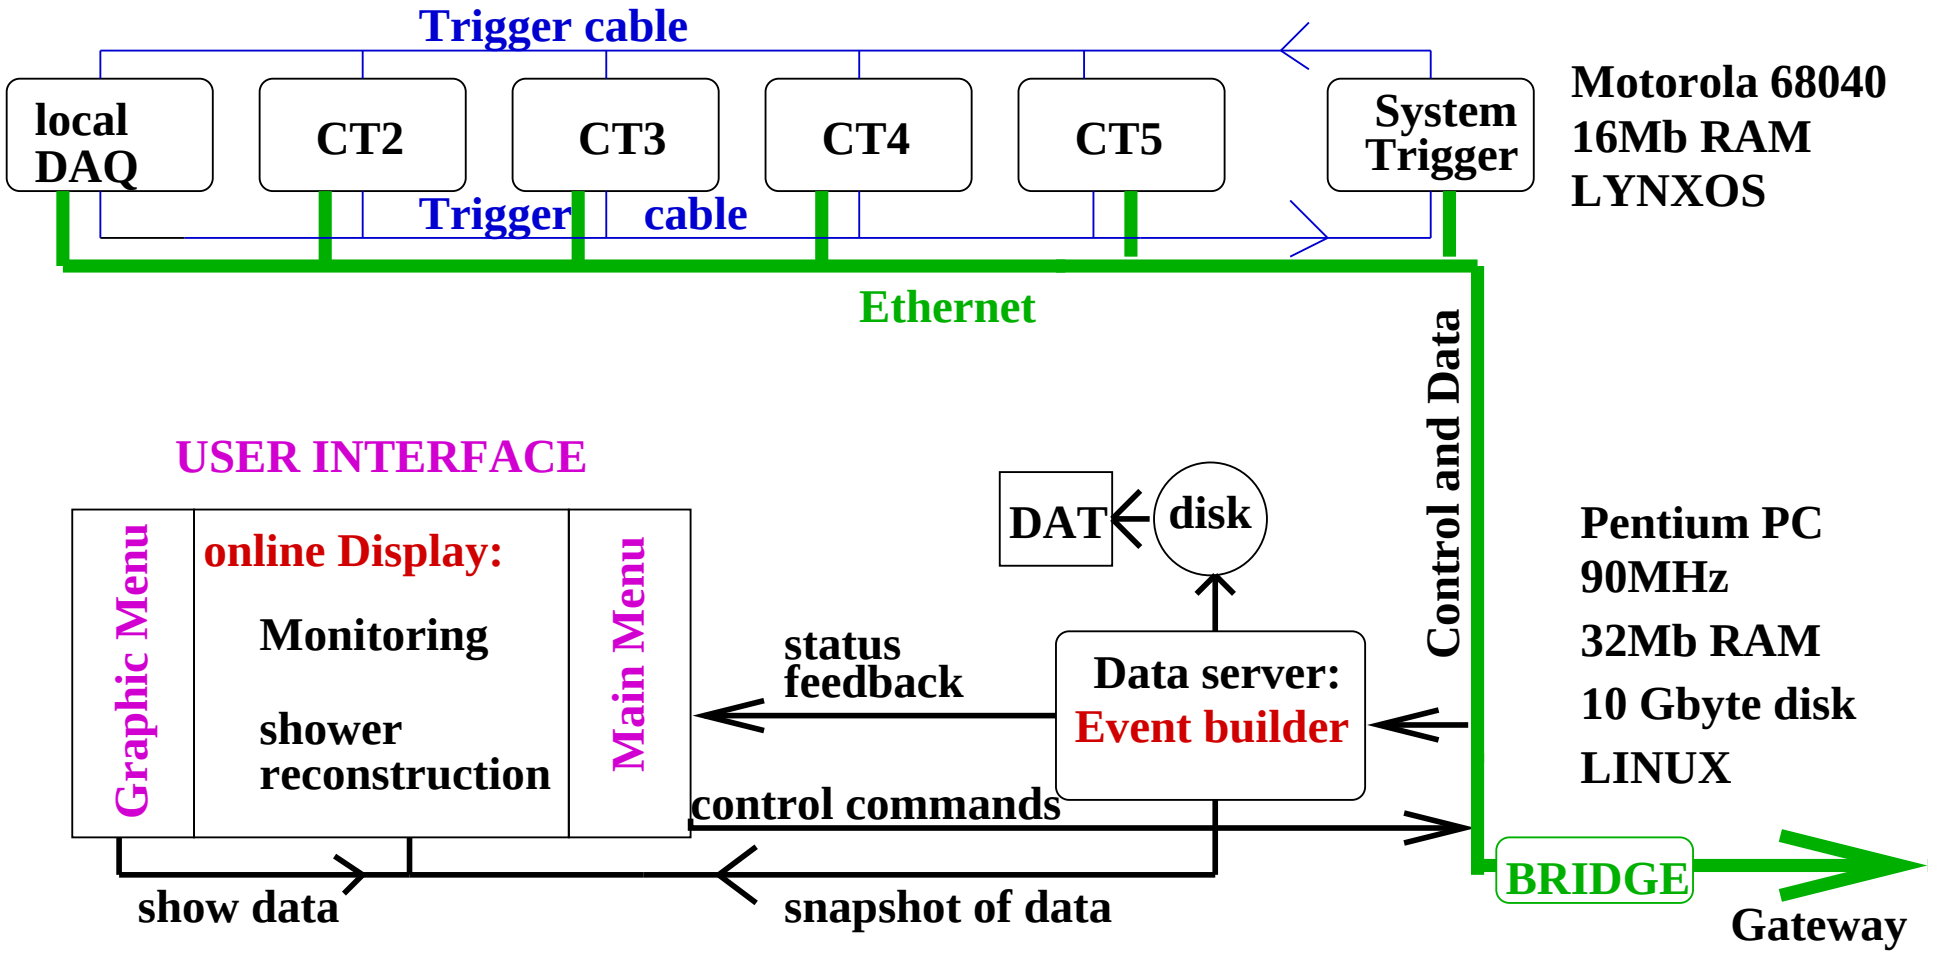Architecture of the DAQ of a 5 CT System